


The multifunction instrument PV CHECKS performs prompt and safe electrical checks required for a PV system (DC section) and controls of the functionality of modules / strings in accordance with IEC/EN62446 guidelines.

PV CHECKS: safety checks

PV CHECKS verifies continuity of protective conductors (and associated connections) and measures insulation resistance of the active conductors on a module, a string, or a photovoltaic field in accordance with IEC/EN62446 guidelines, so avoiding to use any external switch to short-circuit positive and negative terminals.


PV field not connected to ground

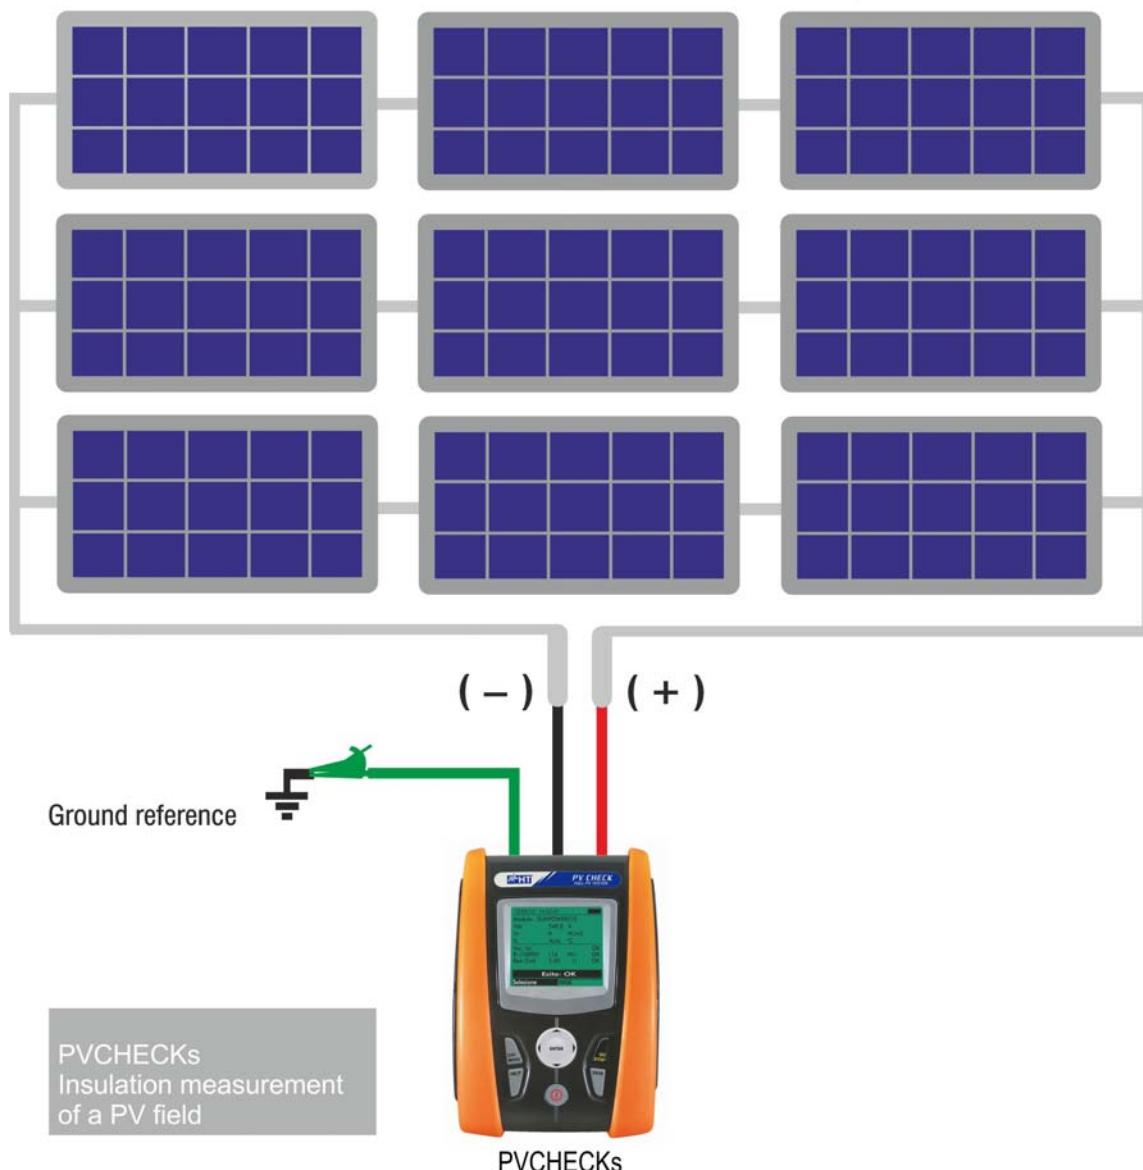

Direct measurement of insulation resistance on a PV Field not connected to ground

PVCHECKS: functionality checks

PVCHECKS verifies functionality of a PV string in accordance with the IEC/EN62446 guidelines by measuring open circuit voltage and short-circuit current under operating conditions up to 15A and extrapolating the results referred to the STC (by measuring the solar radiation). Finally, it displays measurements as well as comparison with the PV strings previously tested.

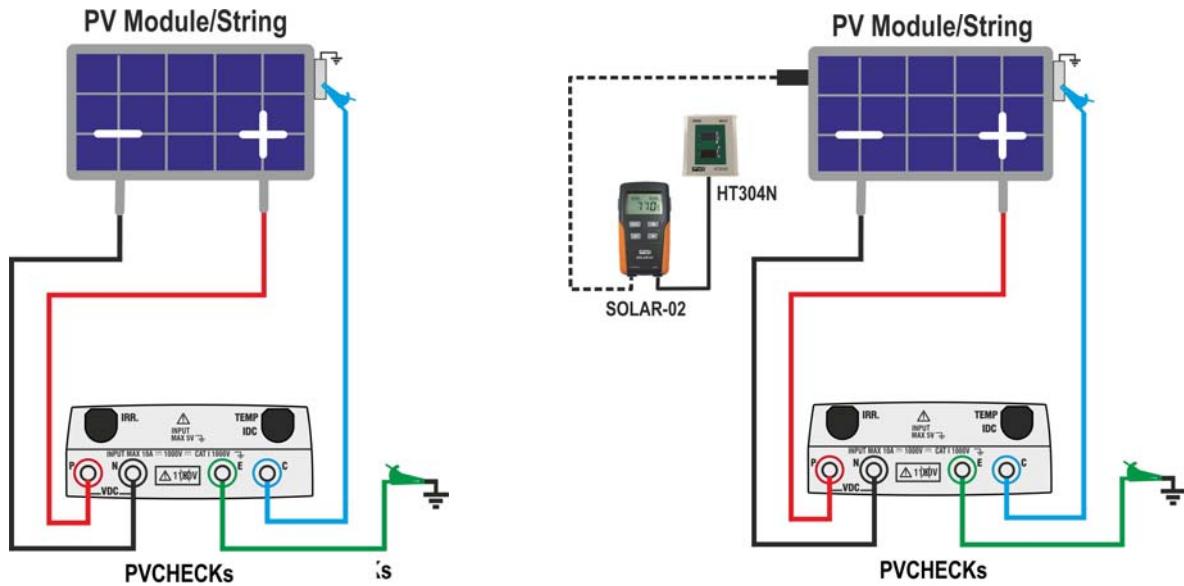


Test IVCK – Automatic measurement of Voc, Isc + Insulation + Continuity on a PV Module/String without irradiance measurement

Test IVCK – Automatic measurement of Voc, Isc + Insulation + Continuity on a PV Module/String with irradiance measurement with optional accessories SOLAR-02 and HT304N

PVCHECKS: performance checks

PVCHECKS analyses the performance of a PV array (DC) under the operating conditions (connected to the inverter) displaying the generated power and the efficiency of the PV plant in accordance with IEC/EN62446.

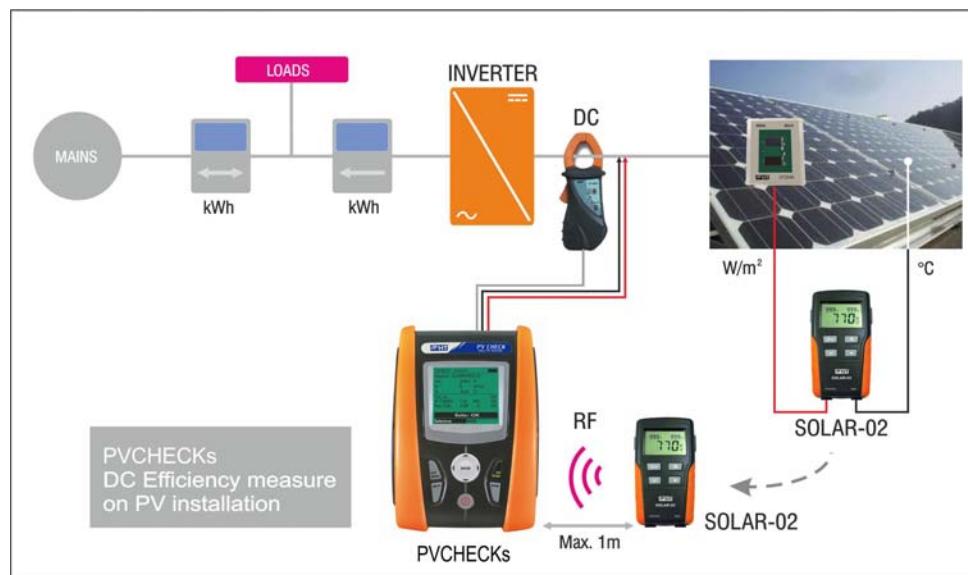



2. ELECTRICAL SPECIFICATIONS

Accuracy is calculated as $\pm [\% \text{ readings} + (\text{no. of digits}) * \text{resolution}]$ at $23^\circ\text{C} \pm 5^\circ\text{C}$, relative humidity <80%HR

2.1. PERFORMANCE TEST

DC Voltage

Range (V)	Resolution (V)	Uncertainty
5.0 ÷ 199.9	0.1	
200.0 ÷ 999.9	0.5	$\pm (1.0\%\text{rdg} + 2\text{dgt})$

DC current (by mean external clamp)

Range (mV)	Resolution (mV)	Uncertainty
-1100 ÷ -5		
5 ÷ 1100	0.1	$\pm (0.5\%\text{rdg} + 0.6\text{mV})$

DC current is always positive ;DC current zeroed if the related voltage value is < 5mV

FS DC clamp [A]	Resolution [A]	Minimum read value [A]
1 < FS ≤ 10	0.001	0.05
10 < FS ≤ 100	0.01	0.5
100 < FS ≤ 1000	0.1	5

DC Power (Vmeas > 150V)

Clamp FS (A)	Range (W)	Resolution (W)	Uncertainty
1 < FS ≤ 10	0.000k ÷ 9.999k	0.001k	$\pm(1.5\%\text{rdg} + 3\text{dgt})$
10 < FS ≤ 100	0.00k ÷ 99.99k	0.01k	$(I_{\text{meas}} < 10\%\text{FS})$ $\pm(1.5\%\text{rdg})$
100 < FS ≤ 1000	0.0k ÷ 999.9k	0.1k	$(I_{\text{meas}} \geq 10\%\text{FS})$

Irradiance (by mean HT304N)

Range (mV)	Resolution (mV)	Uncertainty
1 ÷ 40.0	0.02	$\pm(1.0\%\text{rdg} + 0.1\text{mV})$

Temperature (by mean PT300N)

Range (°C)	Resolution (°C)	Uncertainty
-20.0 ÷ 100.0	0.1	$\pm (1.0\%\text{rdg} + 1^\circ\text{C})$



2.2. FUNCTIONALITY TEST

DC Voltage @ OPC

Range (V)	Resolution (V)	Uncertainty
5.0 ÷ 199.9	0.1	$\pm(1.0\%rdg+2dgt)$
200 ÷ 999	1	

Minimum VPN voltage to start the test: 15V

DC Current @ OPC

Range (A)	Resolution (A)	Uncertainty
0.10 ÷ 15.00	0.01	$\pm(1.0\%rdg+2dgt)$

DC Voltage @ STC

Range (V)	Resolution (V)	Uncertainty
5.0 ÷ 199.9	0.1	$\pm(4.0\%rdg+2dgt)$
200 ÷ 999	1	

DC Current @ STC

Range (A)	Resolution (A)	Uncertainty
0.10 ÷ 15.00	0.01	$\pm(4.0\%rdg+2dgt)$

Irradiance (by mean HT304N)

Range (mV)	Resolution (mV)	Uncertainty
1 ÷ 40.0	0.02	$\pm(1.0\%rdg + 0.1mV)$

Temperature (by mean PT300N)

Range (°C)	Resolution (°C)	Uncertainty
-20.0 ÷ 100.0	0.1	$\pm(1.0\%rdg + 1°C)$



2.3. SAFETY TEST

Continuity Test (LOWΩ)

Range [Ω]	Resolution [Ω]	Uncertainty
0.00 ÷ 1.99	0.01	$\pm(2.0\% \text{rdg} + 2\text{dgt})$
2.0 ÷ 19.9	0.1	
20 ÷ 199	1	

Test current >200mA DC up to 2Ω (test leads included), Resolution 1mA, Uncertainty $\pm(5.0\% \text{rdg} + 5\text{dgt})$

Open loop voltage $4 < V_0 < 10V$

Insulation Test (MΩ) – Mode TIMER

Test voltage [V]	Range [MΩ]	Resolution [MΩ]	Uncertainty
250, 500, 1000	0.01 ÷ 1.99	0.01	$\pm(5.0\% \text{rdg} + 5\text{dgt})$
	2.0 ÷ 19.9	0.1	
	20 ÷ 199	1	

Open voltage: $< 1.25 * \text{nominal test voltage}$

Short circuit current: $< 15\text{mA} (\text{peak})$ for all test voltages

Generated voltage Resolution 1V, uncertainty $\pm(5.0\% \text{rdg} + 5\text{dgt})$ @ Rmis > 0.5% FS

Test current $> 1\text{mA}$ with load = $1\text{k}\Omega \times V_{\text{nom}}$

Insulation Test (MΩ) – Mode FIELD (*), STRING (**)

Test voltage [V]	Range [MΩ]	Resolution [MΩ]	Uncertainty (***)
250	0.1 ÷ 1.9	0.1	$\pm(20.0\% \text{rdg} + 5\text{dgt})$
	2 ÷ 99	1	
500	0.1 ÷ 1.9	0.1	$\pm(20.0\% \text{rdg} + 5\text{dgt})$
	2 ÷ 99	1	
1000	0.1 ÷ 1.9	0.1	$\pm(20.0\% \text{rdg} + 5\text{dgt})$
	2 ÷ 99	1	

(*) For FIELD mode if VPN >1V the minimum voltage VEP and VEN for the calculation of Ri(+) and Ri(-) is 1V

(**) For STRING mode minimum VPN voltage to start the test: 15V

Open voltage <1.25 x nominal test voltage

Short circuit current < 15mA (peak) for each test voltage

Generated voltage resolution 1V, accuracy $\pm(5.0\% \text{reading} + 5\text{digits})$ @ Rmis > 0.5% FS

Rated current measured $> 1\text{mA}$ with $1\text{k}\Omega @ V_{\text{nom}}$

(***) For FIELD mode:

add 5 dcts to the accuracy if
$$\frac{\max\{R^+, R^-\}}{\min\{R^+, R^-\}} \geq 100$$



3. GENERAL SPECIFICATIONS

DISPLAY AND MEMORY:

Features: 128x128pxl custom LCD with backlight
Memory: max 999 test

POWER SUPPLY:

PVCHECK internal power supply: 6x1.5V alkaline batteries type LR6, AA, AM3, MN 1500
Battery life: approx.120 hours (DC efficiency test)
SOLAR-02 power supply: 4x1.5V alkaline batteries type AAA LR03
SOLAR-02 max recording time (@ IP=5s): approx. 1.5h

OUTPUT INTERFACE

PC communication port: optical/USB
Interface with SOLAR-02: wireless RF communication (max distance 1m)

MECHANICAL FEATURES

Size (L x W x H): 235 x 165 x 75mm
Weight (batteries included): 1.2kg

ENVIRONMENTAL CONDITIONS:

Reference temperature: 23°C ± 5°C
Working temperature: 0° ÷ 40°C
Working humidity: <80%HR
Storage temperature (remove the batteries): -10 ÷ 60°C
Storage humidity: <80%HR

GENERAL REFERENCE STANDARDS:

Safety: IEC/EN61010-1
EMC: IEC/EN61326-1
Safety of measurement accessories: IEC/EN61010-031
Measurements: IEC/EN62446 (PV performance, IVCK)
IEC/EN 61557-1, 2, -4 (LOWΩ, MΩ))
Insulation: double insulation
Pollution degree: 2
Overvoltage category: CAT III 300V to ground
Max 1000V DC among inputs P, N, E, C
Max height of use: 2000m

This instrument complies with the requirements of the European Low Voltage Directives 2006/95/EC (LVD) and EMC 2004/108/EC

This instrument satisfies the requirements of 2011/65/EU (RoHS) directive and 2012/19/EU (WEEE) directive

Les services d'EURO-INDEX

EURO-INDEX fournit des services pour tous les instruments de sa gamme de fournitures et offre des services, de la connaissance et du personnel hautement qualifié pour l'entretien (préventif), la réparation et le calibrage de vos instruments de mesure.

Centre de Service Agréé.....

EURO-INDEX est un Centre de Service Agréé pour toutes les marques représentées.

Autrement dit, vos instruments sont traités par du personnel formé et compétent, qui dispose des outils et logiciels adéquats. Seules des pièces d'origine sont utilisées et la garantie de votre instrument ainsi que la certification (ATEX, EN50379, etc.) restent valables.

Laboratoire de maintenance et de calibrage

EURO-INDEX dispose d'un laboratoire de maintenance et de calibrage particulièrement moderne, titulaire d'une accréditation conforme à la norme NEN-EN-ISO/IEC 17025. Cette accréditation est valable pour différentes grandeurs, telles que spécifiées dans le champ d'application associé au numéro d'accréditation K105.



MQS®

MQS est une formule d'entretien exclusive comportant un entretien et un calibrage périodiques de vos instruments de mesure. La prise en charge de multiples aspects vise à vous libérer de tout souci lors de l'utilisation de vos instruments de mesure. Les coûts sont modiques et prévisibles.

Accès numérique à vos certificats de calibrage avec Mon MQS

Mon MQS est un portail Web qui vous donne accès partout et à tout moment à vos certificats de calibrage et aux documents apparentés.

Location d'instruments de mesure

- Vaste assortiment
- Conseils avisés
- Les instruments sont livrés avec leurs accessoires et leurs certificats de calibrage traçables

EURO-INDEX Academy

- Formations sur les produits (individuelles et collectives)
- Séminaires
- Vidéos de démonstration et d'instruction

Visionnez la vidéo sur notre chaîne YouTube et découvrez tout ce qu'il vous faut savoir sur MQS



Guichet des services



Calibrage de l'analyse de gaz de combustion



Séminaires et ateliers



Calibrage de la thermographie

Sous réserve de modifications EURO-INDEX® FR 17001

Le nom et la marque Bluetooth® sont la propriété de Bluetooth SIG Inc. L'utilisation de ce nom par EURO-INDEX s'effectue sous licence.



BELGIQUE

Leuvensesteenweg 607
1930 Zaventem
T: 02 - 757 92 44
F: 02 - 757 92 64
info@euro-index.be
www.euro-index.be

PAYS-BAS

Rivium 2e straat 12
2909 LG Capelle a/d IJssel
T: +31 - (0)10 - 2 888 000
F: +31 - (0)10 - 2 888 010
verkoop@euro-index.nl
www.euro-index.nl



Portée accréditée
voir www.rva.nl

